


VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

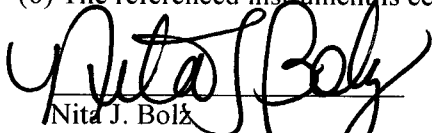
SEP 22 2009

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130286 ✓
Name		Karin Nelson, Sgt	ID# 5349 Date 9/20/09 ✓
A	Agency	North Pole PD	Phone # (907) 488-0412
Instrument Location 125 Shawman Lane, North Pole, AK 99705			
Alco S/N		X172988 ✓	Target Value .080 High Pressure 400 psi
B	Alco Test Values		.079 ✓ 1 st Alco .079 ✓ 2 nd Alco
Signature 			
(OVER)			

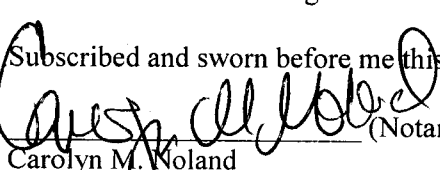
(Do Not write in the area below)

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.


Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 18th day of Oct, 2009.


(Notary Seal Stamp)
Carolyn M. Noland
Notary Public, State of Alaska
Commission Expires with Office



VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130286 ✓

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130286 ✓

SEPTEMBER 20, 2009 ✓ *amb 9/30/09*

OPERATOR'S NAME:

NELSON, KEVIN HOON

OPERATOR'S NUMBER: 5349

SUBJECT'S LAST NAME:

UOC

SUBJECT'S FIRST NAME/MI :

UOC

D.L. #: 00000000

DEPT/AGENCY: NPLI

CASE/REPORT: 09-0000

TEST TYPE: U

ALCO TARGET VALUE: .000 ✓

ALCO S/N: X172988

BREATH ANALYSIS ---
.000 ADJUSTED FOR 29.21 in
ALCO TARGET .078 22:07
BLANK TEST .000 22:08
INTERNAL STANDARD VERIFIED 22:08
ALCO TV 29.21 in .079 ✓ 22:09
BLANK TEST .000 22:09
SUBJECT SAMPLE *amb 9/30/09* .000 22:10
BLANK TEST .000 22:11
ALCO TV 29.21 in .079 ✓ 22:11
BLANK TEST .000 22:12

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130286 ✓

SEPTEMBER 20, 2009 ✓
TIME 22:05

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 01/08/09

HEATERS

SAMPLE CHAMBER: 49c

BREATH TUBE: 41c

BAROMETER: 29.21 in

FLOW DETECTOR: OKAY

HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

!@#%&'()*+,-./0123456789:;<=>?@BCDEF6
HIJ KLMNOPQRSTU VWXYZ[\]^_`abc defghijklmno
pqrstuvwxyz{|}~